



Sofia[®] SARS Antigen FIA



Objective SARS-CoV-2 Results at Your Fingertips



Accurate, objective and automated results in **15 minutes**



Integrated data management automatically stores test and user history



Excellent performance compared to molecular methods



User and patient ID captured with **onboard barcode scanner**




Flexible, dual mode testing for high throughput in variety of laboratory environments



Sofia SARS Antigen FIA – Procedure



Nasal/Nasopharyngeal Swab Procedure

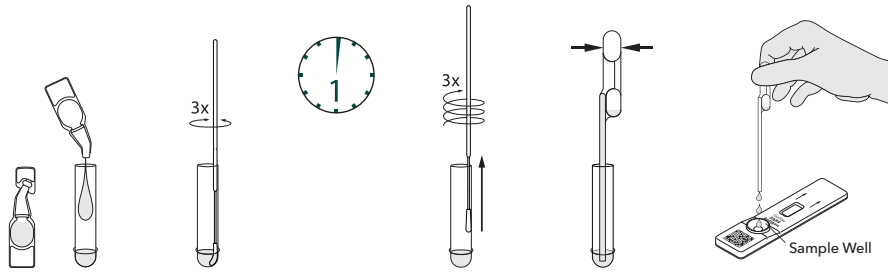

Sofia Development Modes

WALK AWAY Mode – Walk away and multitask

READ NOW Mode – Batch multiple samples per hour

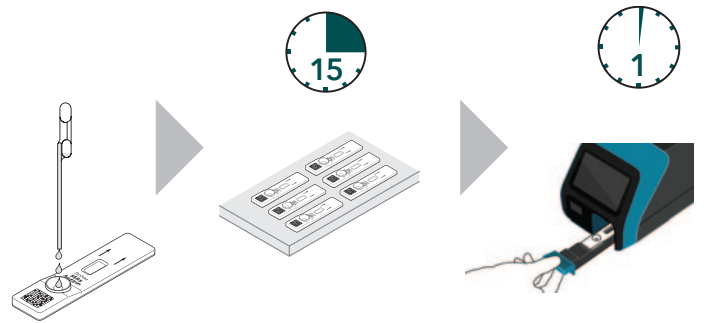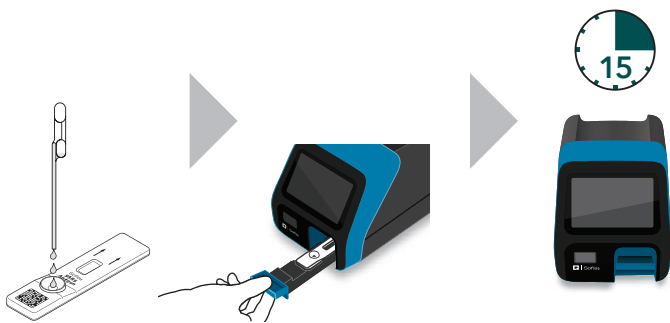

Sofia SARS Antigen FIA

- Nasal and nasopharyngeal specimens
- Accurate detection with direct samples
- Results in 15 minutes
- Kit includes 25 sterile nasal swabs and a set of positive and negative control swabs
- Room temperature storage

	Reference Extracted RT-PCR assay				95% CI			
	POS	NEG	Total	PPA	96.7%	83.3%	99.4%	
Sofia SARS Antigen FIA Assay	POS	29	0	29	NPA	100.0%	97.9%	100.0%
	NEG	1	179	180	PPV	100.0%	88.3%	100.0%
	Total	30	179	209	NPV	99.4%	96.9%	99.9%
				Prevalence	14.4%	7.4%	14.3%	
				% agreement	99.5%			

*Refer to the Package Insert.

POCD

Point of Care Diagnostics

Point of Care Diagnostics Aus. Pty Ltd
 PO Box 4754 North Rocks NSW 2151
 1800 640 075
 admin@pocd.com.au
 www.pocd.com.au



SL3206 | SS20378101EN00 (08/20)

Sofia SARS Antigen FIA – 25 Test Kit: Catalog #20378

